




Anabolic Complex

Sequence :

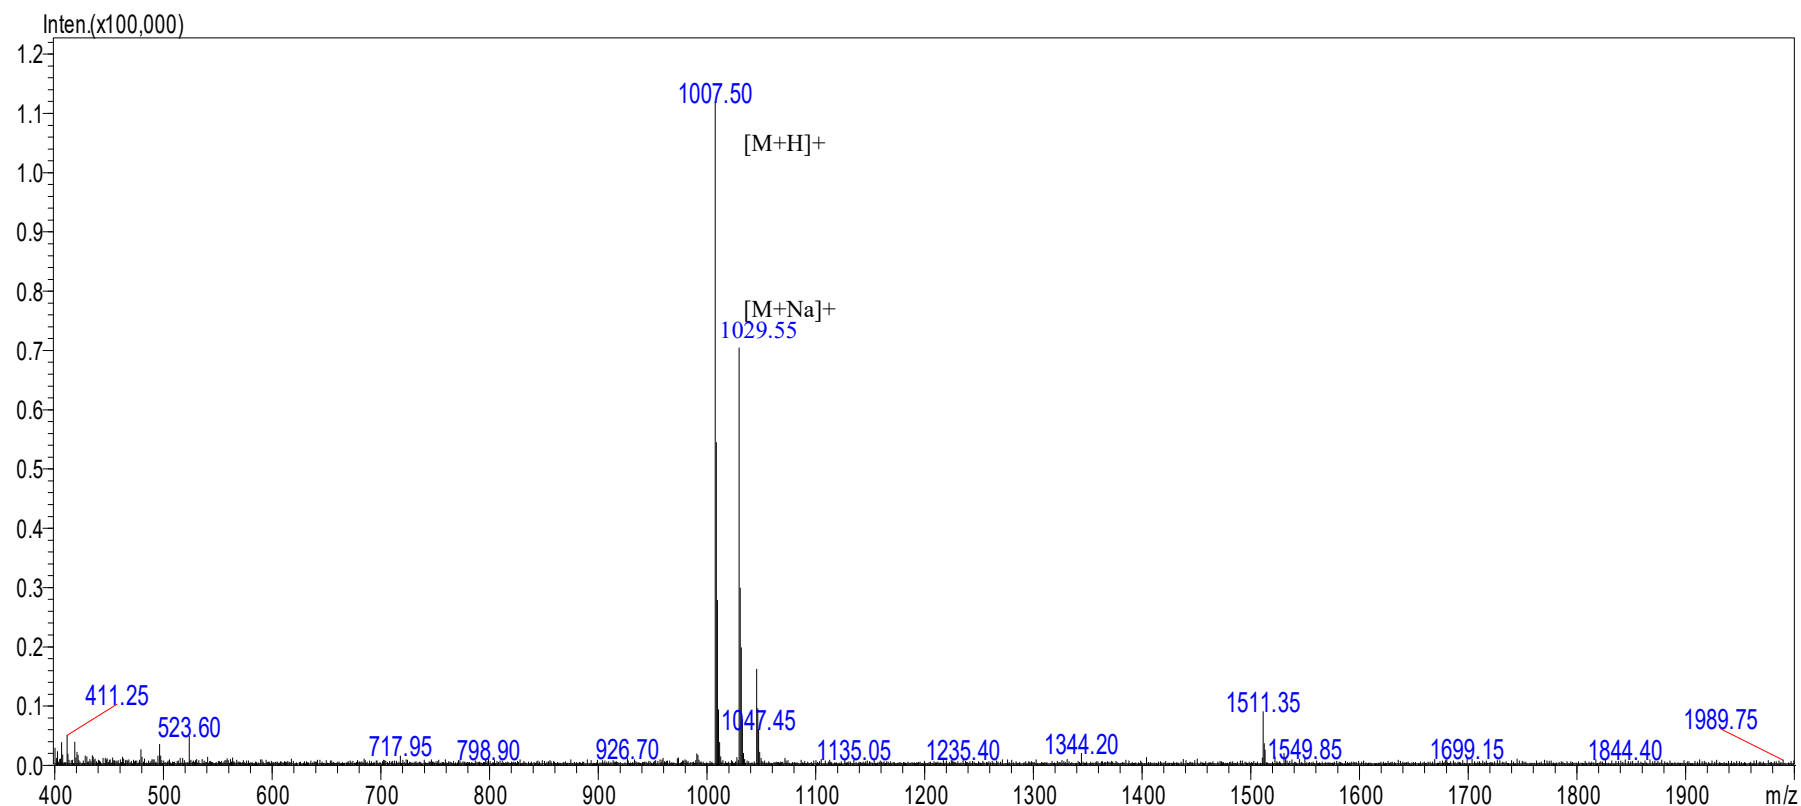

Date and Time: 2019-01-22 16: 30:22
User : CHAO
Sample : Oxytocin Acetate 180515
MW : 1007.2

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN