




### Selank MS Report

[M+H]<sup>+</sup>

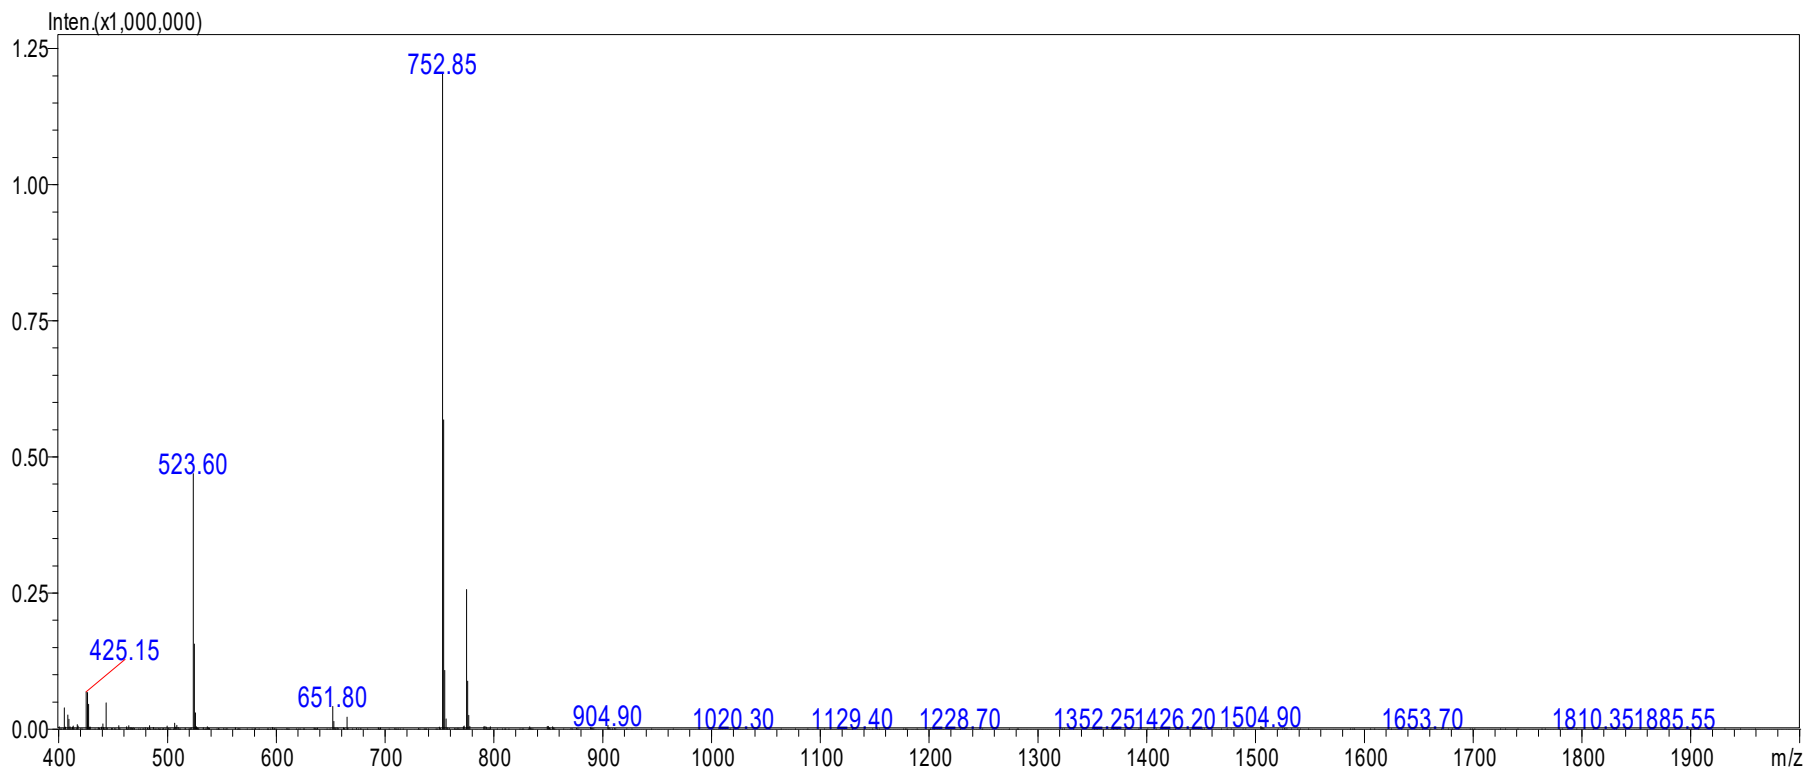

Data Acquired : 2019-01-22 13:25:49  
Injection Volume : 1  
Sample Name : selank  
Mw : 854.99  
Lot No. : P170801-SLN030

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H<sub>2</sub>O/50%ACN