




MASS SPECTROMETRY REPORT

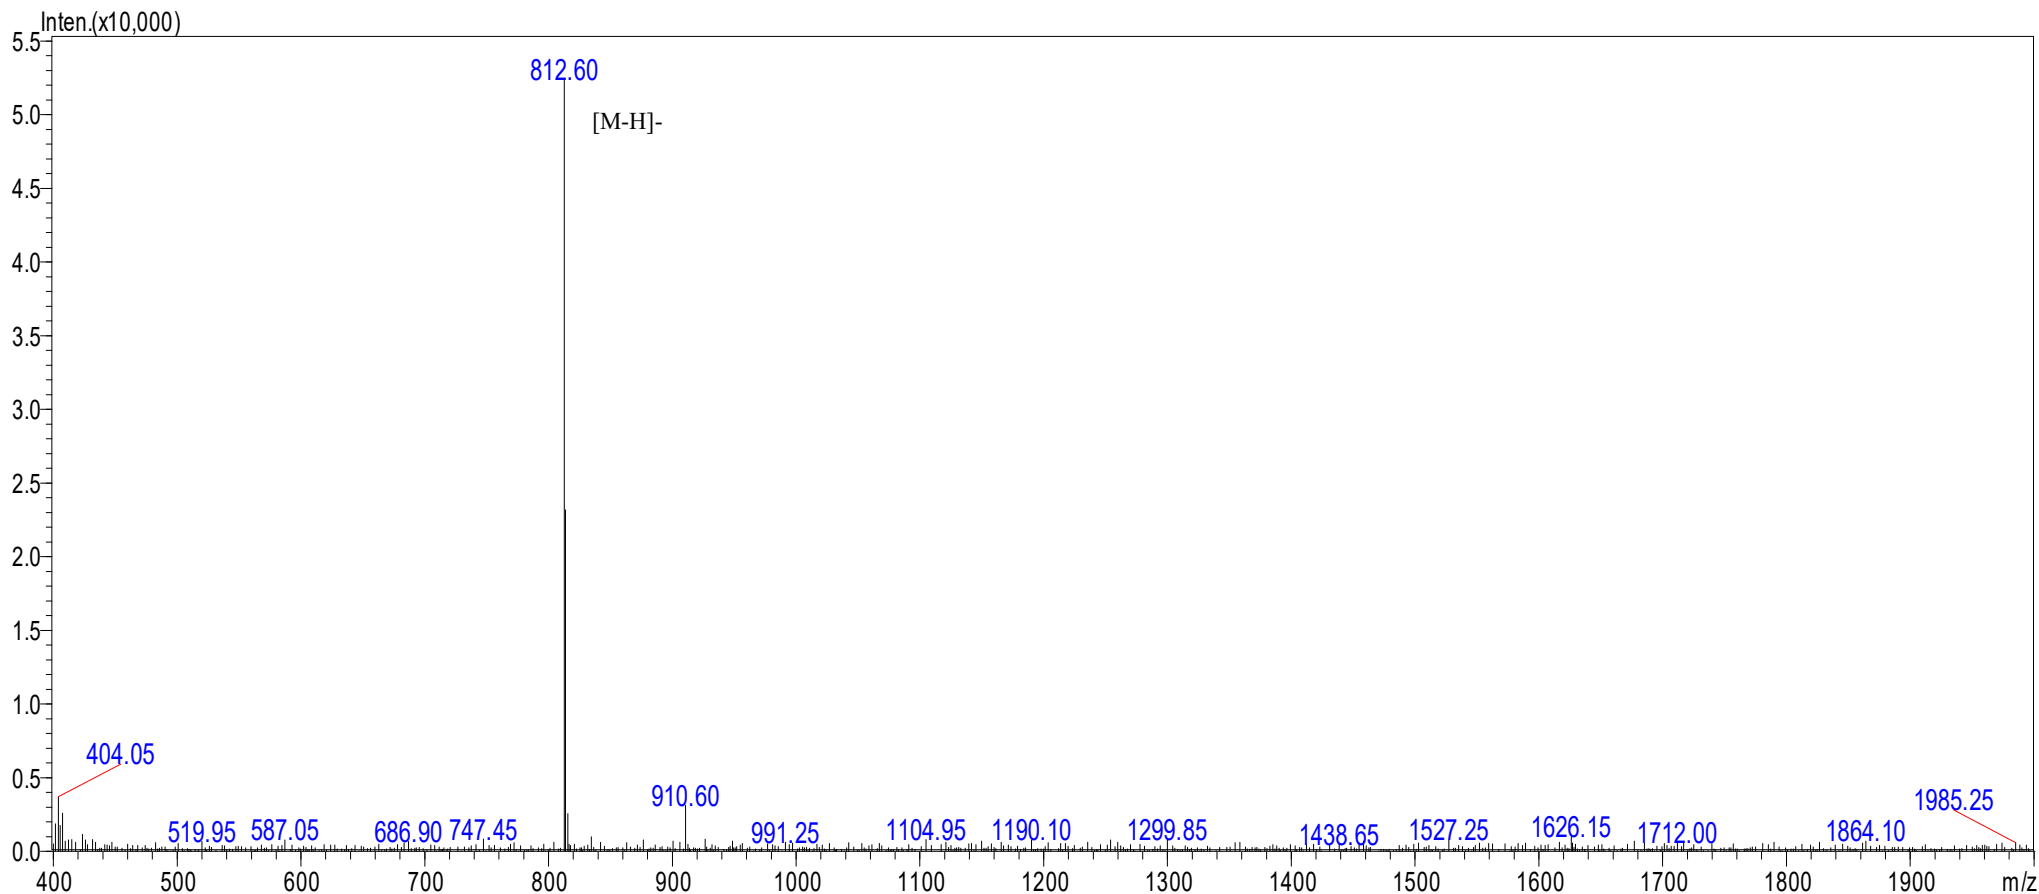

Sample Description

Analyzed date: 2019-01-22
Analyst: SHAO
Sample: semax
M.W.: 813.94
Lot. No.: P171223-LR486110

Instrument

SHIMADZU LCMS-2020
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

SHIMADZU LCMS-2020

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H2O/50%ACN